

GASTEC Instructions for No.109A Oil Mist (Mineral Oils) Airtec Tube

FOR SAFE OPERATION :

Read this manual and the instruction manual carefully.

⚠ CAUTION : If not observed, injuries to the operator or damage to the product may result.

1. When breaking the tube ends, keep away from eyes.
2. Do not touch the broken glass tubes, pieces and reagent with bare hand(s).

△ NOTES : For maintaining performance and reliability of the test result.

1. Use this tube within the temperature range of 0 - 40°C (32 - 104°F).
2. Use this tube within the relative humidity range of 0 - 90%.
3. Oil Mist Airtec Tubes does not react with Synthetic Oil Mist and these types of Oils.
4. Shelf life and storage condition of the tube is marked on the label of the box of tube.

APPLICATION OF THE TUBE :

Use of this tube for the detection of mainly mineral oils, simply connect the pressure reducer to your high pressure air source, compressor, cylinder, or air line and adjust the flow meter to the required setting.

SPECIFICATION :

(As a result of Gastec's commitment to continued improvement, specifications are subject to change without notice.)



	Detecting Layer
Measuring Range	0.3 - 1.5 mg / m ³
Sampling Volume (Flow Meter)	1000 ml
Sampling Rate	1 liter per minute
Sampling Time	60 minutes
Color Change	Yellowish Brown → Greenish Brown
Reaction Principle	Oil Mist + I ₂ O ₅ + H ₂ SO ₄ → I ₂ + CO ₂

**** Shelf Life :** Please refer to the Validity Date printed on the box of tube.

**** Store the tubes in dark and cool place.**

CORRECTION FOR TEMPERATURE, HUMIDITY AND PRESSURE :

Temperature : Temperature correction is not required.


Humidity : Humidity correction is not required.

Pressure : To correct for pressure, multiply the tube reading by


$$\frac{\text{Tube Reading (mg/m}^3\text{)} \times 1013 \text{ (hPa)}}{\text{Atmospheric Pressure (hPa)}}$$

MEASUREMENT PROCEDURE :


1. Install a reducer pressure with gauge and flow meter to a cylinder, compressor or air line and adjust the flow meter the required setting.
2. Break tips off a fresh detector tube in the tube tip breaker and insert a tube into a tube holder.

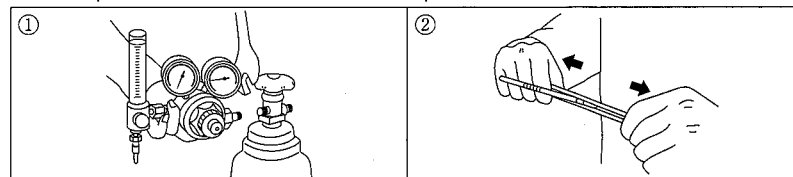

3. Attach the rubber tube holder to the flow meter outlet. Make certain the tube arrow **G** on the tube pointing in a down direction.
4. Turn on the cylinder or compressor and confirm the flow meter according to each Airtec tube specifications. (In case of Compressed Breathing Air Test Kit - Model BA - 1, confirm the reducer gauge over 2.0 kg / cm² and set the reducer on its 1.5 kg / cm² and set the flow meter ball in accordance with each Airtec tube specifications).
5. Time the flow rate with a stopwatch. (Tube 109AD : Flow Meter 1000ml, Time 60 min.)

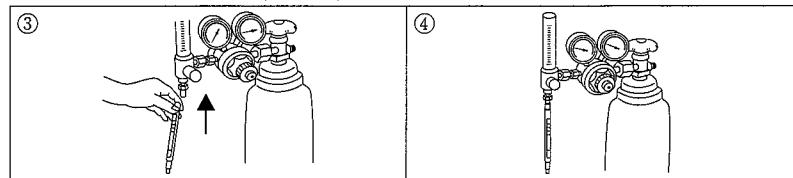

6. As soon as sampling time has elapsed turn off the cylinder or compressor, and remove the tube from the tube holder and then read the colour change layer immediately.

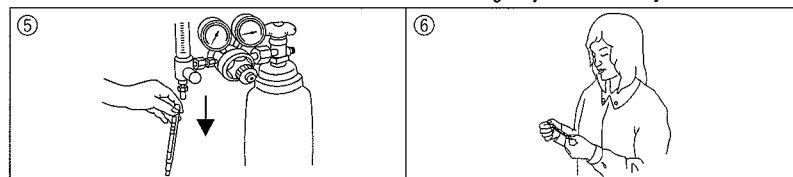

DISPOSAL INSTRUCTION :

Reagent of the tube does not use toxic substance. On disposing the tube regardless of whether used or unused, follow the rules and regulations of the local government.

WARRANTY :

If you have any questions regarding gas detection and quality of the tubes, please feel free to contact your Gastec representatives.

Manufacturer : Gastec Corporation
6431 Fukaya, Ayase-City, 252-1103, Japan

99D - 109A - 1
Printed in Japan