

GASTEC Instructions for No.136LA Methyl Bromide Detector Tube

FOR SAFE OPERATION :

Read this manual and the instruction manual of your Gastec Gas Sampling Pump carefully.

⚠ WARNING:

1. Use only Gastec detector tubes in a Gastec pump.
2. Do not interchange or use non-Gastec parts or components in Gastec's detector tube and pump system.
3. The use of non-Gastec parts or components in Gastec's detector tube and pump system or use of a non-Gastec detector tube with a Gastec pump or use of a Gastec detector tube with a non-Gastec pump may result in property damage, serious bodily injury, and death; voids all warranties; and voids all performance and data accuracy guaranties.

⚠ CAUTION: If not observed, injuries to the operator or damage to the product may result.

1. When breaking the tube ends, keep away from eyes.
2. Do not touch the broken glass tubes, piece and reagent with bare hand(s).
3. The sampling time represents the time necessary to draw the air sample through the tube. The tube must be positioned in the desired sampling area for the entire sampling time or until the flow finish indicator indicates the end of the sample.

△ NOTES : For maintaining performance and reliability of the test results.


1. Use Gastec Gas Sampling Pump together with Gastec Detector Tubes only for the purposes specified in the instruction manual of the detector tube.
2. Use this tube within the temperature range of 0 - 40°C (32 - 104°F).
3. Use this tube within the relative humidity range of 0 - 90%.
4. This tube may be interfered with by the coexisting gases. Please refer to the "INTERFERENCES".
5. Shelf life and storage conditions of the tube are marked on the label of the box of tube.

APPLICATION OF THE TUBE :

Use of this tube for the detection of Methyl Bromide in air or the industrial areas and environmental atmospheric condition.

SPECIFICATION :

(As a result of Gastec's commitment to continued improvement, specifications are subject to change without notice)

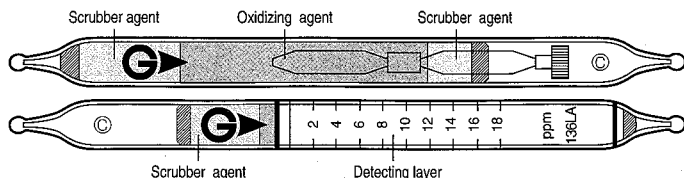

| | | |
|------------------------|---|-------------|
| Measuring Range | 1 - 18 ppm | 18 - 36 ppm |
| Number of Pump Strokes | 2 | 1 |
| Correction Factor | 1 | 2 |
| Sampling Time | 2 minutes per pump stroke | |
| Detecting Limit | 0.2 ppm (n = 2) | |
| Color Change | White → Yellow | |
| Reaction Principle | Methyl bromide produce intermediate product by oxidizing agent and produce yellow stain by reaction with detecting agent. $2\text{CH}_3\text{Br} + \text{I}_2\text{O}_5 + \text{H}_2\text{S}_2\text{O}_7 \rightarrow \text{Br}_2$ $\text{Br}_2 + \text{o-Tolidine} \rightarrow \text{Yellow product}$ | |

Coefficient of Variation : 10% (for 1 to 6 ppm), 5% (for 6 to 18 ppm)

**** Shelf Life : Please refer to the Validity Date printed on the box of tube.**

**** Store the tube in the dark and cool place.**

CORRECTION FOR TEMPERATURE, HUMIDITY AND PRESSURE:

Calibration of the Gastec detector Tube No.136La is based on a tube temperature of 20°C (68°F) and not the temperature of the gas being sampled, approximately 50% relative humidity and normal atmospheric pressure.

Temperature : No correction is required.

Humidity : No correction is required.

Pressure : To correct for pressure, multiply by the tube reading by

$$\frac{\text{Tube Reading (ppm)} \times 1013 \text{ (hPa)}}{\text{Atmospheric Pressure (hPa)}}$$

MEASUREMENT PROCEDURE :

1. For leak checking of the pump insert a fresh sealed detector tube into pump. Follow instructions provided with the pump operating manual.
2. Break tips off a fresh primary tubes and a detector tubes in the tube tip breaker of the pump.
3. Connect © marked ends with rubber tubing after breaking each end.
4. Insert the tube into the pump inlet with arrow (G) on the tube pointing toward pump.
5. Make certain pump handle is all the way in. Align guide marks on pump body and handle.
6. Pull the handle all the way out until it locks on 1 pump stroke (100ml). Wait 2 minutes and confirm the completion of the sampling. Repeat the above sampling procedure one more time.
7. For higher than 18 ppm measurement, prepare fresh tube and take pull 1 pump stroke.
8. Read concentration at the interface of the stained-to-unstained reagent.
9. If correction is needed, multiply the correction factors of pump strokes and pressure.

INTERFERENCES :

| Substance | interference | Changes color by itself to |
|------------------------------------|--------------|----------------------------|
| Chlorine, Bromine, NOx | Plus error | Yellow |
| Saturated halogenated hydrocarbons | Plus error | Yellow |

Carbon tetrachloride and unsaturated hydrocarbons can be removed by the primary tube.

The table of this interference gases primarily expresses the interference of each coexisting gas in the gas concentration range, equivalent to the gas concentration. Therefore, the test result may be given positive result by the other substances not listed in the table. For more information is needed, please contact us or our distributors in your territory.

APPLICATION FOR OTHER SUBSTANCES :

Tube 136La can also be used for other substances as below :

| Substance | Correction Factor | No. of Pump Strokes | Measuring Range |
|--------------------|-------------------|---------------------|-----------------|
| n-Butyl bromide | 1.0 | 2 | 1 - 18 ppm |
| n-Butyl bromide | 2.4 | 1 | 2.4 - 43.2 ppm |
| n-Propyl bromide | 1.0 | 2 | 1 - 18 ppm |
| Chlorobromomethane | 0.7 | 2 | 0.7 - 12.6 ppm |

CORRECTION FACTOR :

Detector tubes are primary designed to measure specific gases. But it is also possible to measure other substances of similar chemical properties with the aid of a correction factor or chart. Therefore, please make use of the correction factor/chart measuring ranges as a reference. For more precise factor please contact your Gastec distributor.

DANGEROUS AND HAZARDOUS PROPERTIES :

Threshold Limit Value-Time Weighted Average by ACGIH (2004) : 1 ppm (7—8hours)

Explosive Range : 10 - 15%

DISPOSAL INSTRUCTION :

Reagent of the tube uses Selenium and Chromic acid as toxic substances. When disposing the tube regardless of whether used or unused, follow the rules and regulations of the local government.

WARRANTY :

If you have any questions regarding gas detection and quality of the tubes, please feel free to contact your Gastec representatives.

Manufacturer : Gastec Corporation
6431 Fukaya, Ayase-City, 252-1103, Japan

IM00136LAE1
Printed in Japan
0411Z